

# SpotOptics


The software people for optics

## OPAL

### AUTOMATED WAVEFRONT SENSOR

#### Single and double pass

- Accurate metrology of standard and aspherical lenses
- Accurate metrology of spherical and flat mirrors
- $\phi=0.3$  to  $\phi=60$  mm
- $\sim F/1$  to  $\sim F/15$
- Accurate motor for z-movement
- Accurate XY and tilt stages for easy centering of lenses

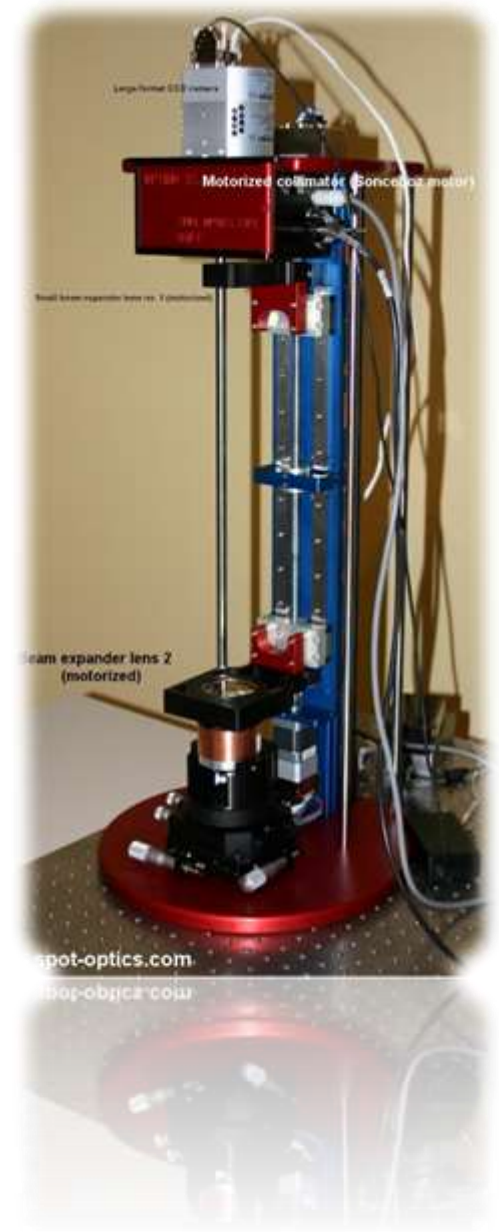

## Technical Specifications

|   |   |
|---|---|
| Measurement Technique                   | Shack-Hartmann wavefront sensor                                 |
| Measurement software                    | Sensoft   |
| Measurement Capability (single pass)    | Wavefronts of small lenses and optical systems in transmission  |
| Measurement Capability (double pass)    | Measurement of reflecting surfaces                              |
| Wavelength                              | White light or any wavelength of choice using a filter          |
| Mounting                                | Vertical  |
| Computer                                | User supplied standard PC. On request, SpotOptics can supply it |
| Software                                | Control and analysis software Sensoft for Windows 8/ Windows 10 |
| <b>TWO MOTORIZED STAGES</b>             |   |
| Motorized Axis                          | Vertical z-axis   |
| Length Measurement                      | Stepper motor with integrated magnetic encoder                  |
| Resolution of stepper motor             | 0.02 $\mu$ m (for a screw with pitch of 1mm)                    |
| Repeatability of home position          | 0.8 $\mu$ m   |
| Measurement range                       | 300mm   |
| Length measurement uncertainty          | 8 $\mu$ m   |
| Speed                                   | Maximum 50 mm/sec   |
| Control software                        | Integrated with analysis software Sensoft                       |
| <b>DIMENSIONS (L x H x D)</b>           |   |
| Size                                    | 600 x 370 x 320 mm (approx)                                     |
| Weight                                  | approx. 20 kg   |
| <b>ACCURACY (all values at 632.8nm)</b> |   |
| Zernike coefficient repeatability       | $\lambda/300$   |
| Measurement Uncertainty                 | $\lambda/20$  |

# Measuring a spherical hemisphere

## Method 1

It is important to note that a high-quality sphere is required to calibrate out the aberrations of the collimator and the OMI system. For practical reasons, it is not possible to have a reference sphere that has an F/# of less than 0.68, which in double pass becomes 1.36 (since the sphere is used at its radius of curvature). This corresponds to **NA=0.37**, covering an angle  $\alpha=21.7^\circ$ . See Table 1, row 1.

## Method 2



Opal can also be calibrated in single pass using a pinhole light source supplied with the instrument. In this case, the limit to the angle  $\alpha$  that can be tested is set by the **NA** of the collimator (i.e.  $\alpha=64.1^\circ$ ). See Table 1, row 2.


## Method

1. Parallel light (coming from Opal) of diameter  $d$  falls on the collimator lens  $C$  of focal length  $f$
2. It comes to focus, and illuminates the hemisphere of diameter  $D_s$  and radius  $R$
3. It then illuminates part of the sphere with diameter  $D$
4. The light is reflected back to the focus, passes through the collimator and is made parallel again. It then illuminates the Shack-Hartmann system of Opal, where it is imaged on the camera after passing through the lenslet array
5. Sensoft then gives the surface error etc.

## Some relations

1. The above figure shows that  $D/R=d/f=1/F\# = 2NA$
2. The angle  $\alpha = n \sin^{-1}(NA)$  is covered by the collimator, where  $n$  (refractive index)=1 (in air)
3. The various collimators that can be used are given in Table 1 below

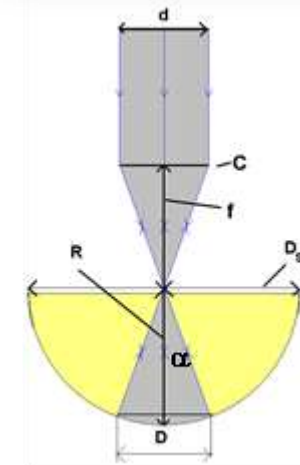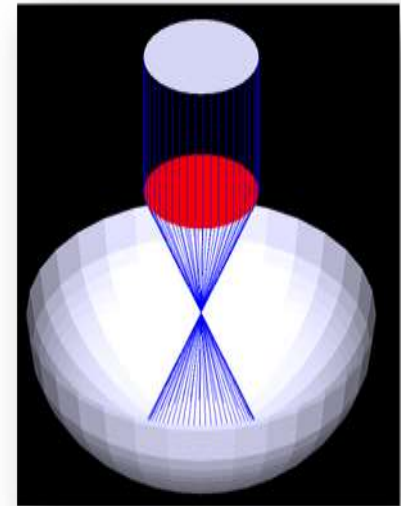

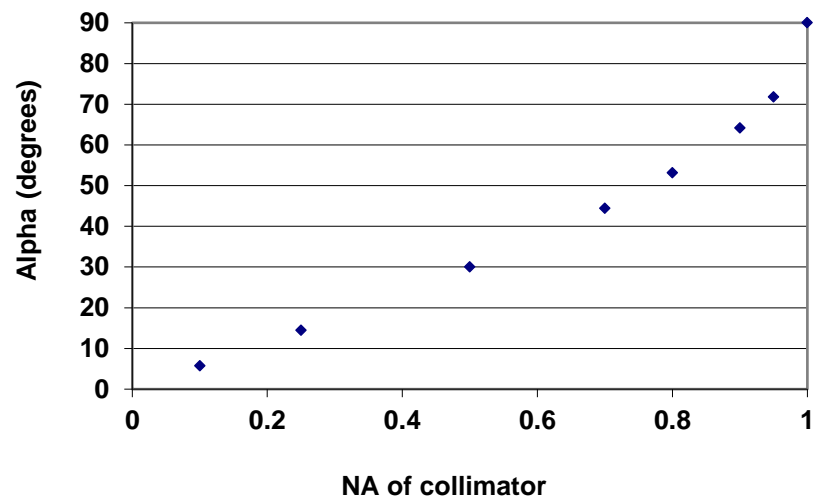

| <b>No.</b> | <b>NA</b>   | <b>Collimator F/#</b> | <b>Angle <math>\alpha</math> covered (deg)</b> | <b>Focal length (mm)</b> | <b>Working distance (mm)</b> | <b>Diameter of output beam (mm)</b> | <b>Number of spots</b> |
|------------|-------------|-----------------------|--|--------------------------|------------------------------|-------------------------------------|------------------------|
| <b>1</b>   | 0.42        | 1.19                  | 24.8   | 10                       | 20                           | 6.6                                 | <b>29x29</b>           |
| <b>2</b>   | <b>0.70</b> | <b>0.71</b>           | <b>64.1</b>                                    | <b>2</b>                 | <b>10</b>                    | <b>3.6</b>                          | <b>18x18</b>           |



## SENSOFT: THE SOFTWARE

### Sensoft: The modular software package:


- Fully controls the hardware of Lentino
- Performs the Shack-Hartmann (SH) analysis
- Computes Zernike coefficients, diagnostics (alignment and correct focal plane), wavefront, MTF, spot diagram
- Has a Loop mode for on-line adjustment of optical system

### Opal in your production line:

- Opal – with its own PC - can easily be adapted to the production line
- It can work in a closed-loop with the PC of the manufacturing machine
- A software module defines the communication protocol and transfers the results between the PCs
- Additional package for remote setup of Opal and communication of output results over the Local Area Network

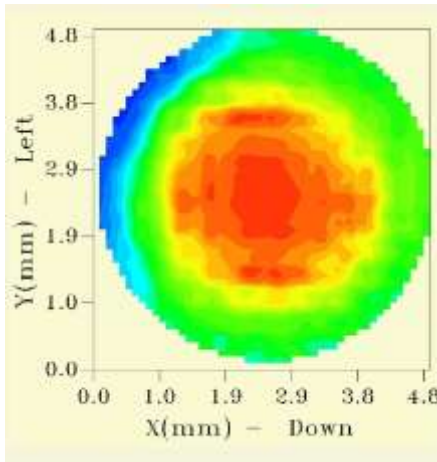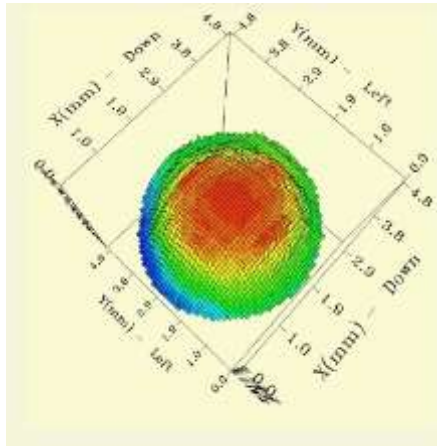


## ON-LINE ALIGNMENT OF COMPLEX OPTICAL SYSTEM IN A FAST LOOP

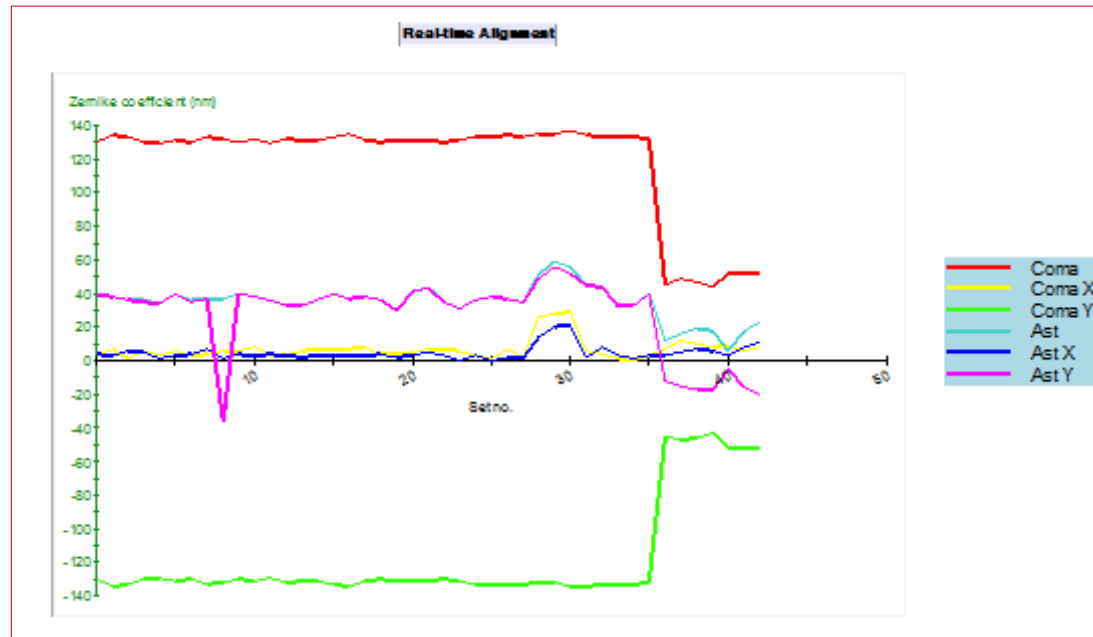

- The alignment of complex optical systems becomes easy by monitoring coma and astigmatism in a continuous loop
- The individual (x, y) components of coma and astigmatism, as well as the total coefficients are displayed
- The optimization can be done for one component at a time, as the software can display one component of interest
- Optimal alignment is reached when the coma and astigmatism components converge towards a given tolerance


# MTF MEASUREMENTS

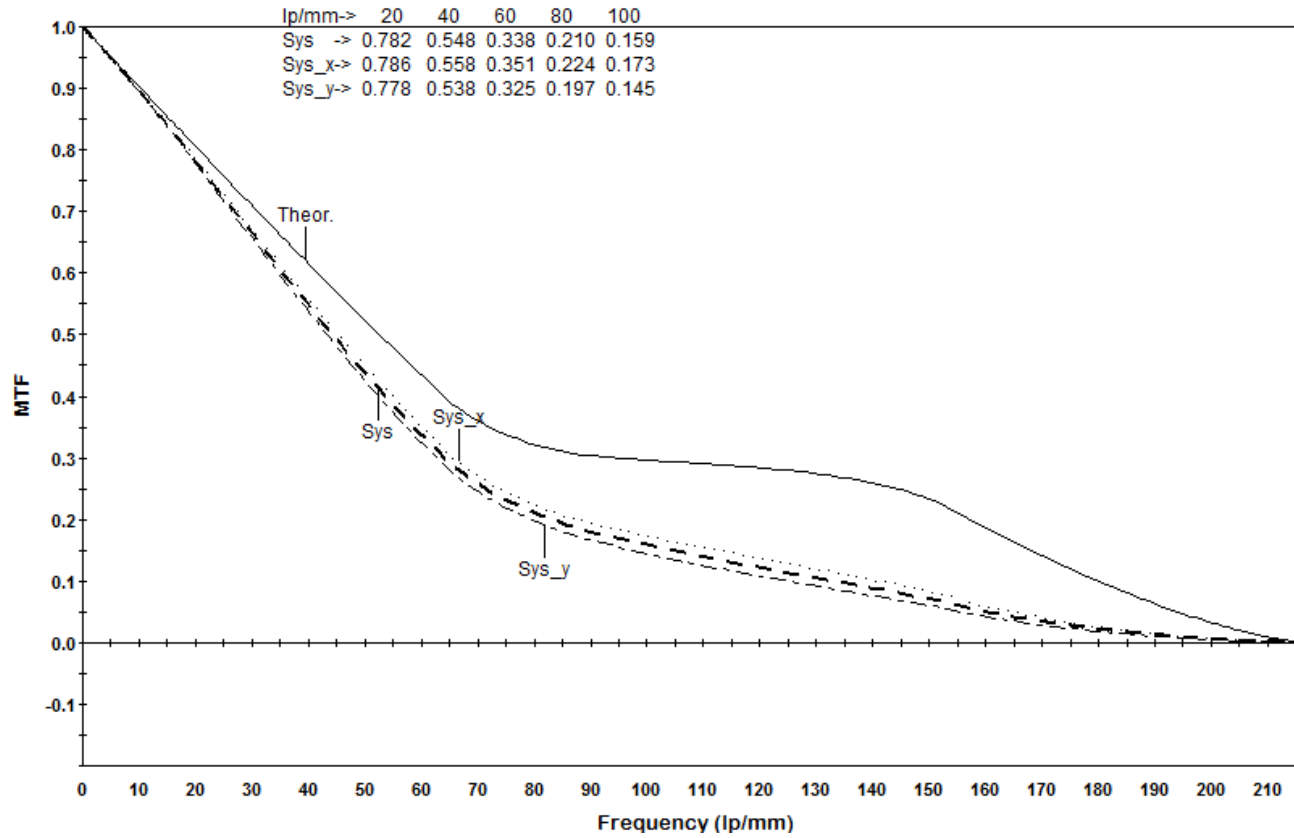

MTF after subtracting the contributions of tilt and defocus present in the data

## The instrument with beam expander

Large format CCD camera. Other cameras available

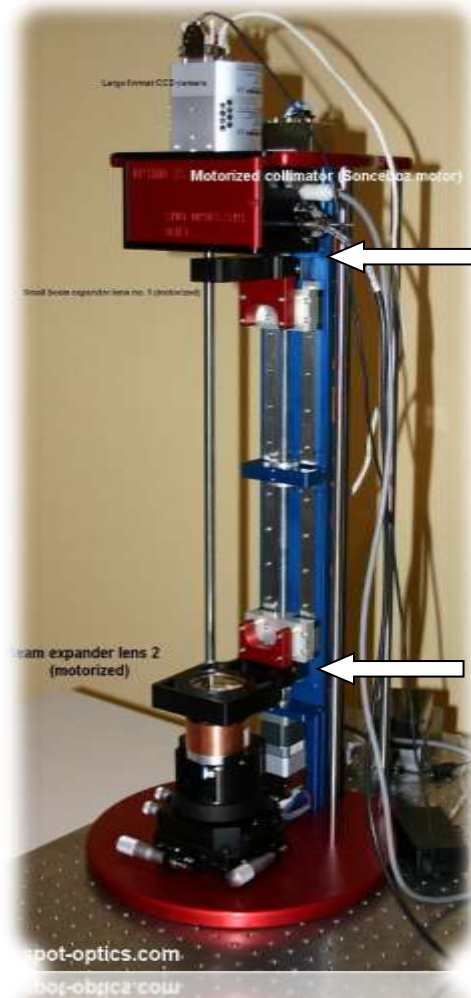

Small beam expander no. 1 (motorized)

Beam expander lens no. 2 (motorized). Up to  $\phi=58\text{mm}$



- Shack-Hartmann wavefront sensor for use in production line and laboratory
- Insensitive to vibrations
- Modular design allows measurement on a variety of surfaces (flat and spherical components)
- Can be used in double pass or single pass, giving flexibility
- Lenses can be tested in transmission using parallel light or pinhole
- Absolute and relative radius of curvature measurements as well as focal length
- Automated measurement
- High-resolution integrated encoder in stepper motor
- Built-in autocollimator for ensuring that the lens mounting is parallel to the axis of OMI